


# MAST<sup>®</sup> CARBA PACe

*Pseudomonas*, *Acinetobacter*, Enterobacterales  
rapid carbapenemase detection

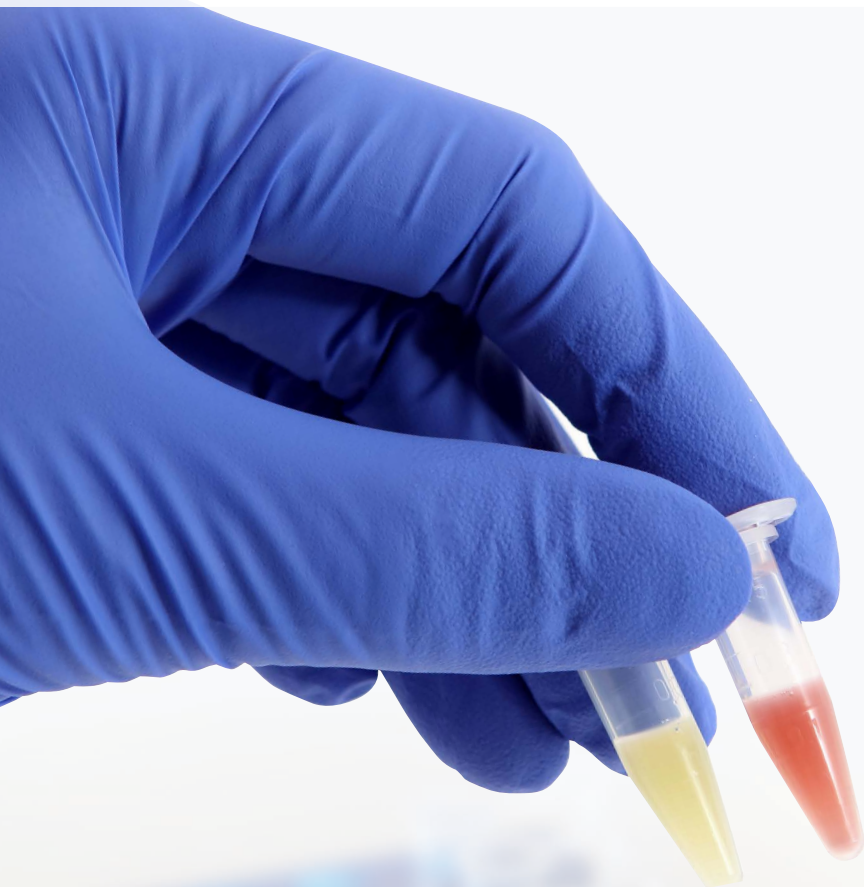

- Rapid results in less than 10 minutes
- Simple test process in 5 easy steps
- Cost effective screening solution
- High sensitivity and specificity

# MAST<sup>®</sup> CARBA PAcE

An increase in antimicrobial resistance is one of the most urgent global challenges facing the field of healthcare. Healthcare associated infections (HAI) are one of the most common adverse effects in care delivery and the occurrences of epidemics of HAI are a major public health problem (WHO 2017).

Carbapenem resistant Gram negative bacteria, including Enterobacterales (CRE), *Pseudomonas aeruginosa* and *Acinetobacter baumannii* are an emerging cause of HAI and accordingly a global public healthcare concern due to high levels of antimicrobial resistance and ability for widespread transmission. It is important to recognise carriers quickly to prevent and control the spread in nosocomial and community settings and also to aid antibiotic stewardship.

## MAST<sup>®</sup> CARBA PAcE

**Mast Group Ltd.** remains at the forefront of the fight against such threats and as such has developed a colorimetric test which rapidly detects carbapenemase producing *Pseudomonas* spp., *Acinetobacter* spp. and Enterobacterales using a novel chromogenic cephalosporin analogue for which there is a patent pending for its application.

The new **MAST<sup>®</sup> CARBA PAcE** is a simple cost effective screening solution providing rapid results within 10 minutes, yet reliable in detecting carbapenemase production to support patient treatment. Additionally, no special equipment is required allowing it to be easily integrated into any laboratory workflows.

The basis of this colorimetric test is the hydrolysis of the chromogenic cephalosporin analogue, eliminating the effects of ESBL and AmpC enzymes using suitable inhibitor compounds, providing specific carbapenemase detection. Therefore only distinguishing epidemiologically significant carbapenem resistance, avoiding patient isolation unnecessarily.


## Benefits of MAST<sup>®</sup> CARBA PAcE

- |  |  |
|--|--|
| <b>Rapid time to result</b>                  | – Once the test organism is added to the test solution results are available within 10 minutes   |
| <b>Cost effective</b>                        | – Conveniently contains 48 tests per kit, allowing rapid identification of carbapenemase producers, assisting with prompt isolation of carriers to prevent cross transmission. |
| <b>Easily integrated into any laboratory</b> | – Requiring only standard microbiological supplies making this adaptable to any laboratory workflows   |
| <b>Easy to Use</b>                           | – Simple test procedure, with 5 simple steps (see figure 1), colour change from yellow to orange/red indicates carbapenemase activity  |
| <b>Quality</b>                               | – Validated using a panel of organisms including VIM, IMP, NDM, OXA-48-like, OXA-23 and KPC high sensitivity and specificity of 96% and 91% respectively                       |
| <b>Supports effective IPC</b>                | – Rapid and reliable detection supports infection prevention and control   |

# MAST<sup>®</sup> CARBA PACe

## Simple test Process

### Reconstitute

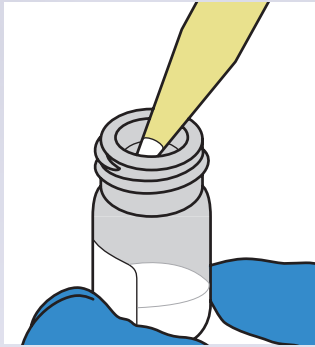

Reconstitute the pellet with 3.6ml of reconstitution buffer.




Allow the pellet to fully dissolve at room temperature for 1 minute and mix contents by gently vortexing for 10 seconds.

### Dispense




Dispense 250µl of reconstituted solution into the tubes provided. One tube per test.


### Inoculate

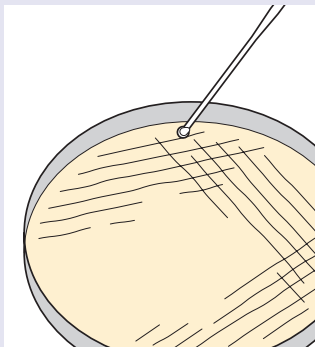

Use a pure, fresh culture of the test organism,

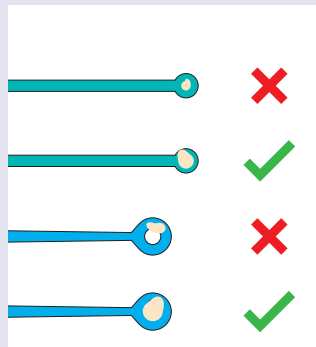

Take an approximate 1 - 5µl loopful of organism, and

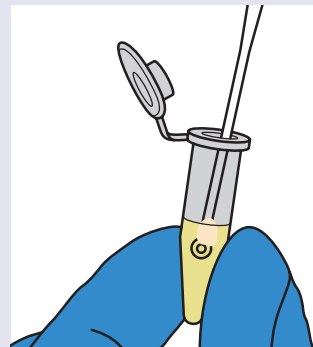


Add to the tube containing test solution



Mix well by vortexing for 20 seconds

### Incubate

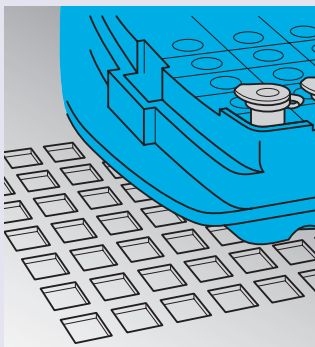

Incubate at 35±1°C for 10 minutes.

### Read by eye



Record the colour of the test solution immediately or up to 20 minutes after incubation 1

## Ordering Information

Order Code	Product	Pack Size	No. Tests
PACE-ID	<b>MAST<sup>®</sup> CARBA PAcE</b> For the rapid detection of carbapenemase producing Enterobacterales, <i>Pseudomonas</i> spp. & <i>Acinetobacter</i> spp.	4 × vial PEL 4 × vial RB	48

## Additional products from Masts AMR range

Order Code	Product	Pack Size	No. Tests
D73C	<b>MASTDISCS<sup>®</sup> Combi Carba plus</b>	5 × 50 discs	50
D72C	<b>MASTDISCS<sup>®</sup> Combi AmpC, ESBL &amp; Carbapenemase Detection Set</b>	6 × 50 discs	50
D74	<b>MAST<sup>®</sup>ICT Indirect Carbapenemase Test</b>	25	25
D71C	<b>MASTDISCS<sup>®</sup> ID CAT-ID - Carbapenemase Activity Test</b>	5 × 50 discs	250

### References

Guidelines for the prevention and control of carbapenem-resistant Enterobacteriaceae, *Acinetobacter baumannii* and *Pseudomonas aeruginosa* in health care facilities. World Health Organisation 2017.

Acute trust toolkit for the early detection, management and control of carbapenemase-producing Enterobacteriaceae (Published: December 2013 PHE publications gateway number: 2013314)

### Acknowledgement

HMRZ compound used in this product was developed by Dr. Hideaki Hanaki of Kitasato, Institute, Japan.

ZT219 v1.0 CA 02/19

**United Kingdom**  
Mast Group Ltd.  
Mast House  
Derby Road, Bootle  
Merseyside L20 1EA

Tel: + 44 (0) 151 933 7277  
Fax: + 44 (0) 151 944 1332  
e-mail: sales@mast-group.com

**Germany**  
Mast Diagnostica GmbH  
Feldstrasse 20  
DE-23858 Reinfeld

Tel: + 49 (0) 4533 2007 0  
Fax: + 49 (0) 4533 2007 68  
e-mail: mast@mast-diagnostica.de

**France**  
Mast Diagnostic  
12 Rue Jean-Jacques Mention  
CS 91106  
80011 Amiens CEDEX 1

Tél. + 33 (0) 322 80 80 67  
Fax + 33 (0) 322 80 99 22  
e-mail: info@mast-diagnostic.fr